MIDMARK®

Installation/Operation Instructions

9A214001/002 RESTRAINT BELTS

KIT COMPONENTS

Part Number	Description	Qty.
053-0148-00	Restraint Belts	2
040-0010-47	Screws (#10-24 x 3/8" Phillips	4
050-1320-00	Belt Mount Brackets	2
003-0751-00	Installation / Operation Instructions	1

REQUIRED TOOLS

Phillips Screwdriver

INTRODUCTION

To restrain patient to table during examination / procedures.

INSTALLATION (BELT MOUNTS)

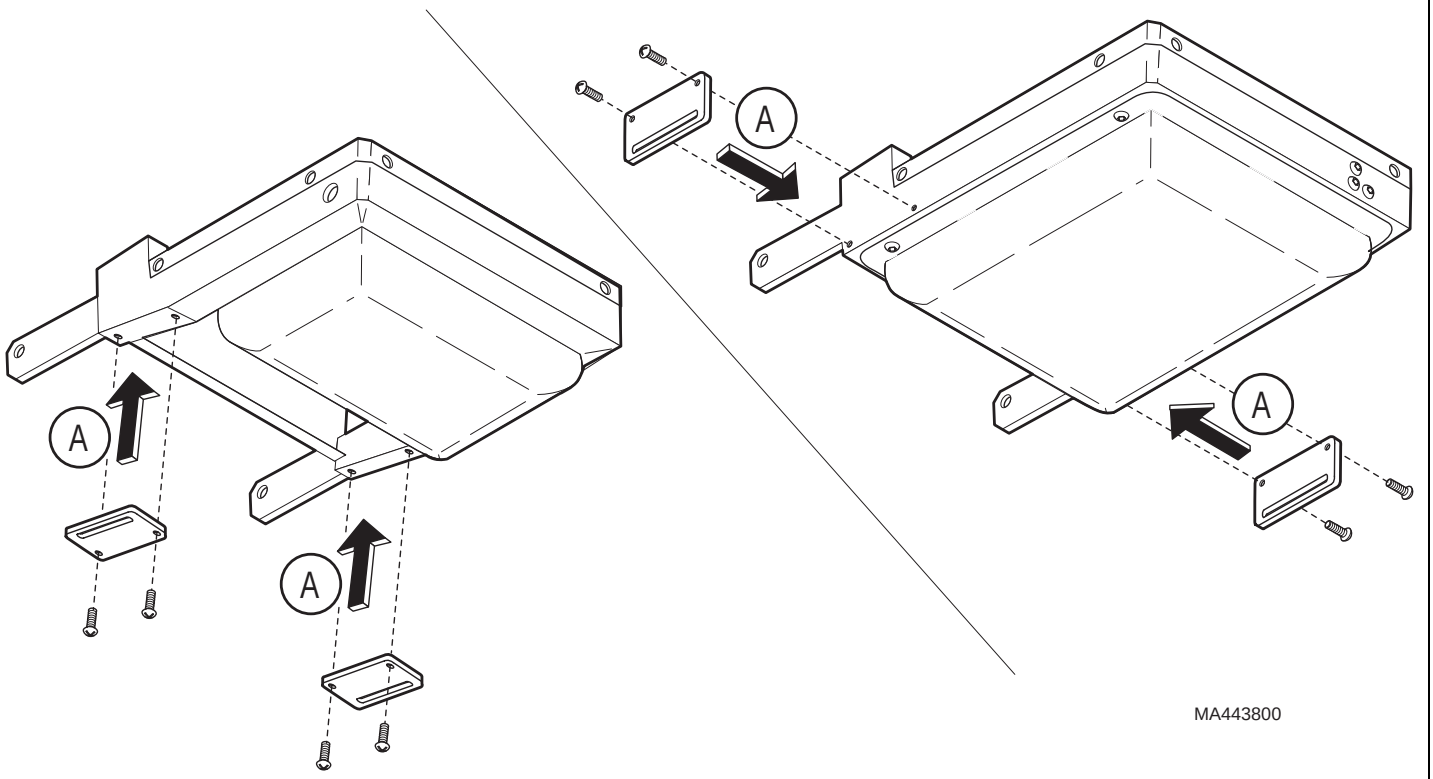

NOTE

For ease of installation raise table and foot rest up and tilt table back.

A. Place belt mounts in position at bottom of foot rest. Secure with mounting screws.

© Midmark Corporation - 1998

INSTALLATION (LEG SECTION)

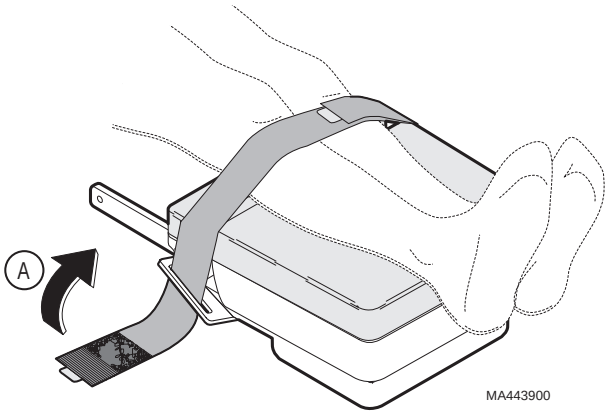

A. Place velcro end of strap through slot of belt mounts, looping it so velcro contacts top of strap.

INSTALLATION (BACK SECTION)

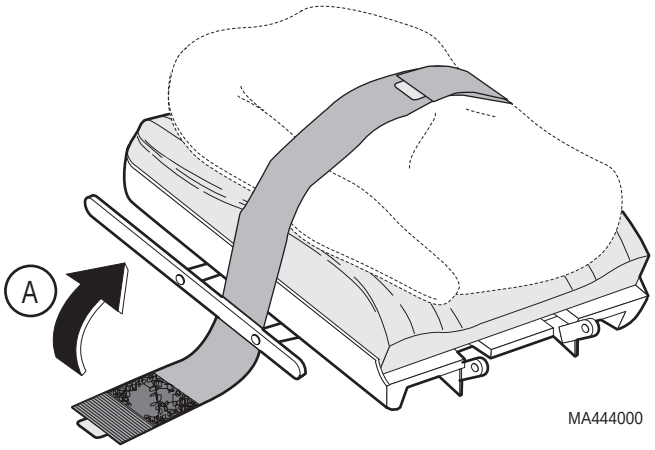

A. Place velcro end of strap through opening between back section and side bar, looping it so velcro contacts top of strap

© Midmark Corporation - 1998